

INSTRUCTIONS FOR USE PIN INDEX MEDICAL GAS REGULATOR



	PAGE
1. SYMBOLS	2
2. INTENDED USE OF DEVICE	2
3. TECHNICAL DESCRIPTION	3
4. WARNINGS	4
5. INSTRUCTIONS FOR USE	5
6. CLEANING AND DISINFECTION	6
7. INSPECTION AND USER CHECKS	6
8. MAINTENANCE	7
9. ACCESSORIES AND SPARE PARTS	7
10. PERFORMANCE	8
11. SERIAL NUMBERS	8
12. INTENDED LIFE	8
13. APPLICABLE STANDARDS	9
14. WARRANTY	10
15. MANUFACTURER AND EU REPRESENTATIVE DETAILS	12
















READ THESE INSTRUCTIONS PRIOR TO USING THIS EQUIPMENT

A COPY OF THESE INSTRUCTIONS CAN BE FOUND ON OUR WEBSITE (WEB ADDRESS STATED ON THE BACK PAGE OF THIS BOOKLET)

CHECK THERE IS NO DAMAGE TO THE DEVICE PRIOR TO OPENING AND USING. IF ANY DEFECTS FOUND PLEASE NOTIFY THE MANUFACTURER OR AUTHORISED REPRESENTATIVE.

1. SYMBOLS

	Indicates a potentially hazardous situation which could result in injury to the user or others, if not avoided.
	Read these instructions before using the equipment
	Do not use any form of grease or oil
	No Smoking
	Do not use this device near any source of ignition
	Product part number
	Serial Number
	Manufactured by
	Date of manufacture and country of manufacturer.
	Use-by date
	Storage and operating temperatures.
	Authorised Representative details
	Medical Device

2. INTENDED USE OF DEVICE

There are two main uses for the Meditech range of Medical Gas Regulators.

Units fitted with a pressure outlet, typically 4 bar, are used to provide gas to a device which requires an input at this pressure. Primarily, pneumatically powered medical devices such as a ventilator or Demand Valve. The pressure outlet is supplied in accordance with a national or international standard and there is the potential for a second pressure outlet for use with another item. The second outlet may be to the same national or international standard as the first, or it may be different.

Units fitted with a flow outlet are used to deliver variable flow rates of gas to a patient who requires gas therapy. The patient will be breathing on his own but may have a need for

support to supply oxygen enriched air to increase blood oxygen levels. The flow outlet will be either a 'fir tree connector' for use with standard oxygen tubing fitted to a therapy mask, or canula or a threaded outlet for use with a humidifier. Flow outlets can be switched between different rate in the range of 0.5lpm (litres per minute) to 15 lpm, with an optional 'MAX' setting of approximately 25lpm used for system purging.

Units are available with both a pressure outlet and a flow outlet and these can be used for either purpose or both simultaneously.

Note: This IFU is referring to the use of oxygen throughout. However, the same instructions apply for the different gas type regulators available from B.N.O.S. Meditech. These include Medical Air 4, Medical Air 7, Nitrous Oxide, N₂O/O₂ Mixed gas, and Carbon dioxide regulators.

3. TECHNICAL DESCRIPTION

This manual refers to B.N.O.S. Meditech 55B and 55SL medical gas regulators with pin index input fittings.

55B Range regulators are designed for mobile use in demanding conditions. The main material of manufacture is brass. They are also suitable for use in static conditions.

55SL Range regulators are designed for mobile use where light weight is important. The main material of manufacture is aluminium alloy, but with a brass high pressure Medical Gas path for safety. They are also suitable for use in static conditions.



Figure A: Pin Indexed Regulator.

Key to components

- a. Regulator body
- b. Pressure gauge
- c. Yoke
- d. Yoke Screw
- e. Yoke Sealing Washer
- f. Pin Index
- g. Output Quick Connection
- h. Probe Quick Connection
- i. Therapy Mask Elastomeric Connection
- j. Therapy Outlet from Regulator
- k. Therapy Outlet Flow Selector
- l. Therapy Outlet Flow Display Window

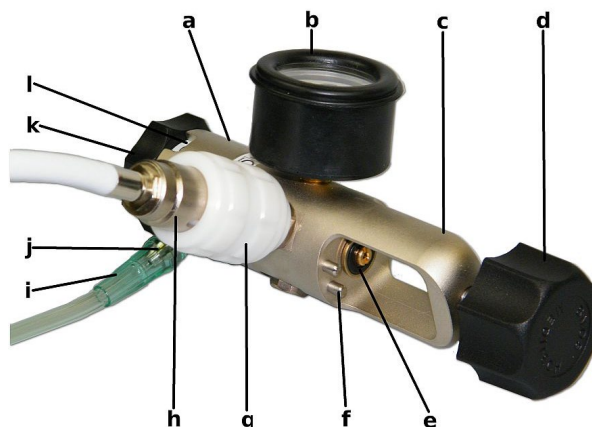
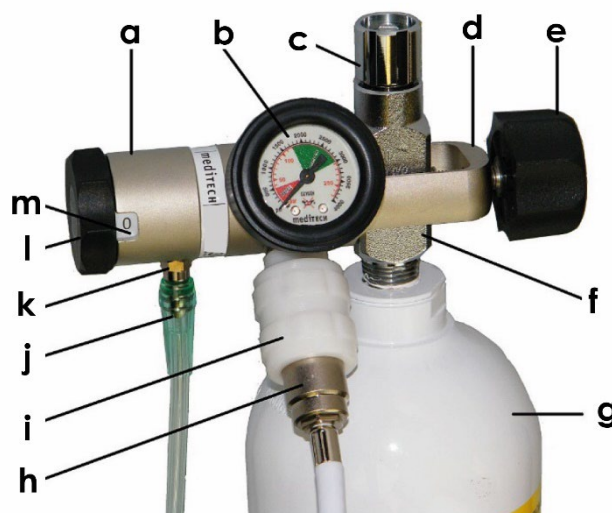


Figure B: Pin Indexed Regulator assembled to Medical Gas Cylinder

Key to components

- a. Regulator body
- b. Pressure gauge
- c. Medical Gas Cylinder Valve
- d. Yoke
- e. Yoke Screw
- f. Medical Gas Cylinder Valve Body
- g. Medical Gas Cylinder
- h. Probe Quick Connection
- i. Output Quick Connection
- j. Therapy Mask Elastomeric Connection
- k. Therapy Outlet from Regulator
- l. Therapy Outlet Flow Selector
- m. Therapy Outlet Flow Display Window



4. WARNINGS!



THIS MEDICAL GAS REGULATOR IS TO BE USED BY ADEQUATELY TRAINED PERSONNEL ONLY.



- 4.1 The user should ensure that no grease, oil, or other contaminants come into contact with the cylinder, valve, regulator, gauge(s), flow selector or connections to mitigate risk of fire.
- 4.2 Do not use this device near any source of ignition e.g., naked flame, electrically powered heaters, cigarettes etc.
- 4.3 Always open the cylinder valve **slowly** to minimise pressure shocks.
- 4.4 The connectors fitted to the Regulator are designed specifically for this device. If replacements are needed, they must be approved parts supplied by B.N.O.S. Meditech Ltd.
- 4.5 The Regulator must not be disassembled when it is under pressure, as serious injury could result.
- 4.6 The Therapy Outlet Flow Selector (if fitted) must be set at the defined settings shown on the dial. It must not be set between adjacent settings, as this may result in no flow from the outlet.
- 4.7 The accuracy of the Therapy Outlet Flow selector (if fitted) will be affected if the input pressure is varied from the nominal value shown in the Performance section of this document.
- 4.8 Note that increasing output flow is obtained from the Therapy Outlet Flow selector (if fitted) if the control is turned clockwise.
- 4.9 The setting of the Therapy Outlet Flow selector (if fitted) does not indicate that a flow is occurring. The User must check that medical gas is flowing to the patient by another means.
- 4.10 Attention is drawn to the accuracies stated in the Performance section of this document.
- 4.11 Do not use the flow outlet for driving any medical equipment.
- 4.12 The use of the regulator for gases other than that on the device labelling is prohibited.
- 4.13 Do not attempt to modify the fittings to suit other gases or fitting systems.
- 4.14 Do not use this device past the use-by date specified on the labelling (This is 10 years from manufacture). Or if the device is found to be not performing as per mandatory inspection and user checks.
- 4.15 This device is dedicated only for use with the gas specified on the label. Never try to use with another gas.
- 4.16 Before connecting any accessory or medical device to the regulator, always check that its fully compatible with the product connection features and the product performances.
- 4.17 When connecting any accessory, the flow outlet make sure that it's not connected to the patient before operating the product.

5. INSTRUCTIONS FOR USE

(EXAMPLE IN PICTURE IS SHOWING A BS SCHRADER (BS 5682) TYPE. THIS MAY VARY IF USING INTERNATIONAL FITTINGS)

5.1. ATTACHING TO A CYLINDER

- 5.1.1 Inspect the Pin Indexed Regulator (Fig: A) and check that the Yoke sealing washer (e) is in place and in serviceable condition.
- 5.1.2 Check your Medical Gas Cylinder to ensure that it is correctly labelled and the correct Medical Gas. Ensure that any new gas cylinders are fitted with a tamper evident seal. Remove all traces of the seal. The Index Pins (f) prevent incorrect attachment of the wrong type of gas cylinder and will locate only into the two matching holes on the face of the corresponding type of Medical Gas cylinder valve.
- 5.1.3 Position the Regulator Yoke (Fig: B) (c) over the Cylinder valve body (n), having first loosened the Yoke Screw (d). Position the Index Pins (f) into their locating holes and tighten Yoke Screw (d) securely, ensuring that the Pressure Gauge (b) and Outlets (g and j) are in the correct orientation. We recommend the orientation shown in Figure B where the output quick connection (g) is close to the Medical Gas cylinder body (m). During assembly ensure the regulator gauge is not compressed against the cylinder valve, which can damage the gauge and prevent the Yoke sealing washer functioning. When the assembled regulator and cylinder is placed in the kit bag, the cylinder gauge (b) and therapy outlet flow display window (l) can be easily seen and the cylinder valve key (o), output quick connection (g) and Therapy outlet flow selector operated.
- 5.1.4 Open the Cylinder Valve (k) slowly (i.e., facing away from the operator or other personnel) by means of the Cylinder Valve Control (o). If gas escapes around the Yoke sealing washer, turn off cylinder with the Cylinder Valve Control (o) and tighten the Yoke Screw (d). Again, slowly open the cylinder valve, if no gas leak is heard, open the Cylinder Valve one full turn and check that the Pressure Gauge (b) shows that the cylinder is full.
- 5.1.5 If a leak of gas is still heard, turn off the Cylinder Valve and remove the Regulator. Remove and replace the Yoke sealing washer (Fig: A) (e) and repeat from step 5.1.1.
- 5.1.6 To attach a Medical Gas-powered device to the Regulator, insert male Probe (fig A) (h) which is attached to the supply hose into the female Outlet (g) by pushing firmly into the orifice. The coupling will lock automatically.
- 5.1.7 To attach equipment to the therapy outlet (j), connect with elastomeric tubing. When connected select the required flow rate by rotating the Therapy outlet flow selector (k) and observing the flow rate selected in the Therapy outlet flow display window (l).
- 5.1.8 After use the cylinder valve should be turned off.
- 5.1.9 The Therapy outlet flow selector (k) should always be left in the off position ("0" indicated in the Therapy outlet flow selector window (l)) when the therapy outlet is not in use. This prevents Medical Gas escaping un-noticed from the outlet (j) when the Medical Gas bottle is turned on.

5.2. TO CHANGE A USED CYLINDER

- 5.2.1 Turn off the Cylinder Valve (Fig: B) by the Cylinder Valve Control (o)
- 5.2.2 De-pressurise the regulator by operating the therapy flow or equipment connected to the Outlet (e). The pressure gauge (b) reading will move to zero. Turn the therapy flow to the off position ("0" indicated in the Therapy outlet flow selector window (l)) Uncouple the Probe by twisting the knurled collar on the female Outlet (e) in a clockwise direction **IF** using a BS Schrader outlet. The male probe will automatically disconnect.
NOTE: If another outlet type of international fitting is used this may require another force (e.g., pull) different to the BS Schrader of twisting clockwise to disconnect.
- 5.2.3 Unscrew the Regulator Yoke Screw (d) and remove the empty Cylinder ensuring the Yoke sealing washer (Fig: B) (e) remains in place on the regulator.
- 5.2.4 Repeat the instructions for "Attaching to a cylinder". (Section 5.1)

6. CLEANING AND DISINFECTION

- 6.1 Surface cleaning of the regulator should be carried out using soap flakes in solution when disconnected from the gas supply. Never immerse the regulator in any fluids.
 - 6.2 For disinfection purposes a chlorine dioxide-based product (e.g., the Tristel Wipes System) should be used, at a nominal concentration of 0.02% wt./vol. The concentration refers to chlorine dioxide in water. The regulator should be wiped clean only and should not be submerged in any fluids.
 - 6.3 After cleaning or disinfection, the regulator should be wiped with clean water to remove any residue and then allowed to dry before returning to use.
- NOTE:** Pressure regulators are not suitable for autoclaving.

7. INSPECTION AND USER CHECKS

7.1 INSPECTION

- 7.1.1 The regulator should be inspected for damaged or broken components and contamination after each use. Check that the Pressure Gauge (b), Power Output (g) and Therapy Outlet (j) (if fitted) are all tight and undamaged. Check that any controls operate correctly and that the Yoke Screw (d) operates smoothly.
- 7.1.2 If contaminated, the Regulator should be cleaned in accordance with Section 6.
- 7.1.3 If damaged, the Regulator should be withdrawn from service and returned to B.N.O.S. Meditech for assessment and repair.

7.2 USER CHECKS (to be carried out before and after cleaning). Ensure no blockages of the pressure relief valves (frozen in extreme temperature).

- 7.2.1 Connect the regulator to a suitable Medical Gas cylinder. Check the pressure gauge (b) reads zero. Slowly open the cylinder valve. Check the pressure gauge indicates that there is pressure in the cylinder. If it continues to read zero, use a cylinder known to contain gas at a minimum pressure of 50 bar.
- 7.2.2 Check for audible leaks when the therapy outlet flow selector (k), if fitted, is in the off position (0 indicated in the therapy outlet flow selector window (l)).
- 7.2.3 For regulators with a Therapy Outlet Flow Selector, check that the operation of the selector (k) has distinct stops at all settings but can be operated smoothly between settings without undue force. Check that the Medical Gas output increases progressively as the control is operated from 0 to 15 (or MAX). Check there is no flow when the selector is returned to 0.
- 7.2.4 Connect an appliance (e.g., a resuscitator) to the Power Output (g). Check that the appliance is capable of being operated from the Power Output (i.e., Medical Gas is being supplied to it) and that there is no audible leakage from the connector. Disconnect the appliance. Check that the connector operates correctly during the connection and disconnection process.
- 7.2.5 Close the cylinder valve.
- 7.2.6 If the Regulator fails any of these checks, it should be withdrawn from service and returned to B.N.O.S. Meditech Ltd. for assessment and repair.

8. MAINTENANCE

- 8.1 No servicing is needed apart from the inspection tests before use that are mandatory.
- 8.2 Performance should be checked by the user at a minimum on a five-yearly basis, using suitable test equipment. The dynamic and static regulator pressure should be measured at the Power Output, using a Medical Gas cylinder with a minimum content of 75 bar. Verify that the flow rates on all settings are within specification at room temperature. If required, B.N.O.S. Meditech Ltd. can advise on suitable test equipment.
- 8.3 A leak test should also be performed by applying a Medical Gas compatible leak test solution to all outlets, fittings, and joints, where applicable.
- 8.4 B.N.O.S. Meditech Ltd. offers training and certification on the service, repair, and preventative maintenance of Meditech products.

9. ACCESSORIES AND SPARE PARTS

No specific accessories are listed for the Regulator. Spare parts that are replaceable by the end user are as follows:

Protective boot for pressure gauge	633-0027-00
Yoke sealing washer (also known as bodock seal)	033-1021-00

Additional parts are available to medical engineers. Contact the manufacturers for details.

10. PERFORMANCE

Rated maximum upstream pressure (P1): 200 bar

Rated outlet pressure (P2): 4 bar (7 bar variant available for Medical Air)

Test inlet pressure (P3): 8 bar

Standard discharge (Q1): 50 lpm (litres per minute)

Variation of outlet pressure (P2) when inlet pressure is varied from P1 to P3 at a flow of Q1: 4%

For regulators with a Therapy Outlet Flow Selector, the figures represent the flow rate from the "Therapy outlet" in litres per minute (lpm). These figures are subject to a tolerance of $\pm 20\%$ of each stated value or $\pm 30\%$ of each stated value for flows of 1,5l/min or less. If the Therapy Outlet Flow Selector has a MAX setting, this has a nominal flow rate of 25 lpm.

Temperature ranges: Storage: -40°C to $+60^{\circ}\text{C}$
Operating: -20°C to $+60^{\circ}\text{C}$

11. SERIAL NUMBER

The Serial No. is to be found on the "barrel" label of the regulator. It consists of four sections the first letters expressing the general type of device, followed by numbers for the month and year of manufacture and lastly a set of up to five numbers representing the "number" of the unit and differentiating units built in the same month.

Example for Therapy Regulators:

SN	RT Regulator Therapy	03 Month of Manufacture	21 Year of Manufacture	12345 Number of Unit
-----------	--------------------------------	-----------------------------------	----------------------------------	--------------------------------

Example for Non-Therapy Regulators:

SN	R Regulator	03 Month of Manufacture	21 Year of Manufacture	12345 Number of Unit
-----------	-----------------------	-----------------------------------	----------------------------------	--------------------------------

12. INTENDED LIFE

This Regulator has been designed for the demands of the pre-hospital emergency medical market to give many years of reliable service. The regulator is manufactured from the finest quality materials with individual components subject to strict quality control tests to ensure high standards under ISO 13485. The regulator is designed to have a product life span of 10 years (from the manufacturing date), excluding abuse to the instrument. This is specified use-by date on the label with the month and year of expiry as the example shown below.



At the end of the 10-year intended life the product must be withdrawn from service.

Disposal should follow the healthcare setting guidelines.
We reserve the right to change design without prior notice.

13. APPLICABLE STANDARDS

B.N.O.S. Meditech Ltd. is an ISO 13485:2016 certified company.

B.N.O.S. Meditech Regulators are supplied in conformity under a quality system to meet Medical Devices Directive 93/42/EEC and The Medical Devices Regulations UK MDR 2002 (SI 618) as subsequently amended by the EU Exit Regulations of 2019 (SI 791) and 2020 (SI 1478).

The above conformity routes have been inspected by the Notified Body Ref: CE 2797 being BSI, Say Building, John M. Keynesplein 9, 1066 EP Amsterdam, The Netherlands and for UKCA by UK Approved Body UKCA 0086 being BSI, Kitemark Court, Davy Avenue, Milton Keynes, MK5 8PP

Regulators are classified as Class IIb Medical Devices.

The following National & International Standards apply to the device:

Standard Number:	Title:
BS EN ISO 10524-1:2019/A1:2023	Pressure regulators for use with medical gases – Part 1: Pressure regulators and pressure regulators with flow-metering devices
BS 5682:2015 OR International Fittings (if applicable)	Specification for probes (quick connectors) for use with medical gas pipeline systems
BS EN ISO 407:2021	Small medical gas cylinders-Pin index yoke-type valve connections
BS EN ISO 15001:2011	Anaesthetic and respiratory equipment. Compatibility with oxygen
BS EN ISO 15223-1:2021	Medical devices – Symbols to be used with medical device labels, labelling and information to be supplied
EN ISO 20417:2021	Medical devices. Information to be supplied by the manufacturer.

14. WARRANTY

IMPORTANT NOTICE

Manufacturer's Warranty is for a period of 7 years and includes parts and labour. It does not include transport costs.

The responsibility and cost of returning and collecting the unit from the manufacturer or their authorised representative is the owners.

Any disassembly of the regulator beyond that detailed in this manual will invalidate the warranty and the manufacturers disclaim any liability for products that have undergone unauthorised repair.

BLANK PAGE



COMPANY CONTACT DETAILS

This regulator is designed and manufactured by:



B.N.O.S. Meditech Ltd.
9 Fifth Avenue, Bluebridge Ind. Est.,
Halstead, Essex CO9 2SZ, England
Tel: +44 (0)1787 479475,
Fax : +44 (0)1787 477747
E-mail : sales@meditech.uk.com
www.meditech.uk.com



EU REPRESENTATIVE :
MEDICAL DEVICE MANAGEMENT LTD
BLOCK B, THE CRESCENT BUILDING
NORTHWOOD, SANTRY
DUBLIN 9, D09 C6X8
IRELAND
Tel: +353 (0) 1893 4143

CE
2797

UK
CA
0086